



US009227326B2

(12) **United States Patent**
Brewer et al.

(10) **Patent No.:** **US 9,227,326 B2**
(45) **Date of Patent:** **Jan. 5, 2016**

(54) **REMOTE CENTER OF MOTION
MECHANISM AND METHOD OF USE**

USPC 74/490.03-490.05; 600/427;
901/15-16, 23; 606/1, 130
See application file for complete search history.

(75) Inventors: **Reuben D. Brewer**, Millbrae, CA (US);
J. Kenneth Salisbury, Jr., Mountain
View, CA (US)

(56) **References Cited**

(73) Assignee: **The Board of Trustees of the Leland
Stanford Junior University**, Palo Alto,
CA (US)

U.S. PATENT DOCUMENTS

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 334 days.

5,397,323	A	3/1995	Taylor et al.
5,515,478	A	5/1996	Wang
5,630,431	A	5/1997	Taylor
5,817,084	A	10/1998	Jensen
5,890,396	A	4/1999	Kaneko et al.
5,907,664	A	5/1999	Wang et al.
6,047,610	A	4/2000	Stocco et al.
6,246,200	B1	6/2001	Blumenkranz et al.
6,645,196	B1	11/2003	Nixon et al.
6,665,554	B1	12/2003	Charles et al.
6,723,106	B1	4/2004	Charles et al.
7,021,173	B2	4/2006	Stoianovici et al.

(21) Appl. No.: **13/572,452**

(22) Filed: **Aug. 10, 2012**

(Continued)

(65) **Prior Publication Data**

US 2013/0039732 A1 Feb. 14, 2013

FOREIGN PATENT DOCUMENTS

Related U.S. Application Data

JP H04-13578 1/1992
SU 1303150 A1 4/1987

(60) Provisional application No. 61/522,530, filed on Aug.
11, 2011.

(Continued)

(51) **Int. Cl.**

A61B 17/00 (2006.01)
B25J 18/00 (2006.01)
B60R 22/03 (2006.01)
A61B 19/00 (2006.01)
A61M 5/00 (2006.01)
B60R 22/02 (2006.01)

Primary Examiner — Gary Jackson
Assistant Examiner — Scott T Luan
(74) *Attorney, Agent, or Firm* — Shay Glenn LLP

(52) **U.S. Cl.**

CPC **B25J 18/00** (2013.01); **A61B 17/00**
(2013.01); **A61B 19/22** (2013.01); **A61M 5/00**
(2013.01); **B60R 22/03** (2013.01); **A61B**
19/2203 (2013.01); **B60R 2022/021** (2013.01)


(57) **ABSTRACT**

According to one exemplary embodiment, a manipulator device includes a base, first and second linear slides, a drive link, a drive member, a driven member and an end effector. The elements of the manipulator device cooperate to constrain the end effector to rotate about a remote center of motion that is displaced from a proximal center of motion as the drive link moves a carriage of the second linear slide along an arcuate path.

(58) **Field of Classification Search**

CPC ... A61B 17/00; A61B 19/22; A61B 19/2203;
A61M 5/00; B25J 18/00

18 Claims, 13 Drawing Sheets

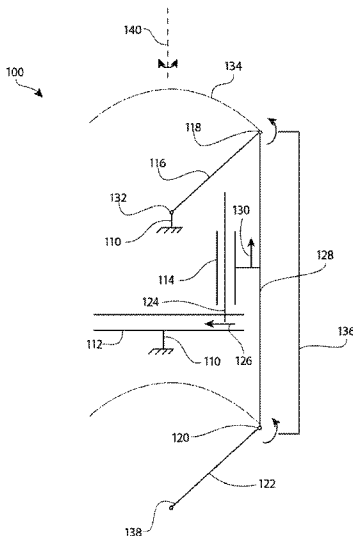

(56)

References Cited

2012/0152050 A1* 6/2012 Richardson 74/490.02

U.S. PATENT DOCUMENTS

FOREIGN PATENT DOCUMENTS

2006/0106345 A1* 5/2006 Flaker et al. 604/131
2008/0262513 A1* 10/2008 Stahler et al. 606/130
2010/0121347 A1 5/2010 Jaspers
2011/0282351 A1 11/2011 Cooper et al.

WO WO2010/122563 A1 10/2010
WO WO2010/130817 A1 11/2010

* cited by examiner

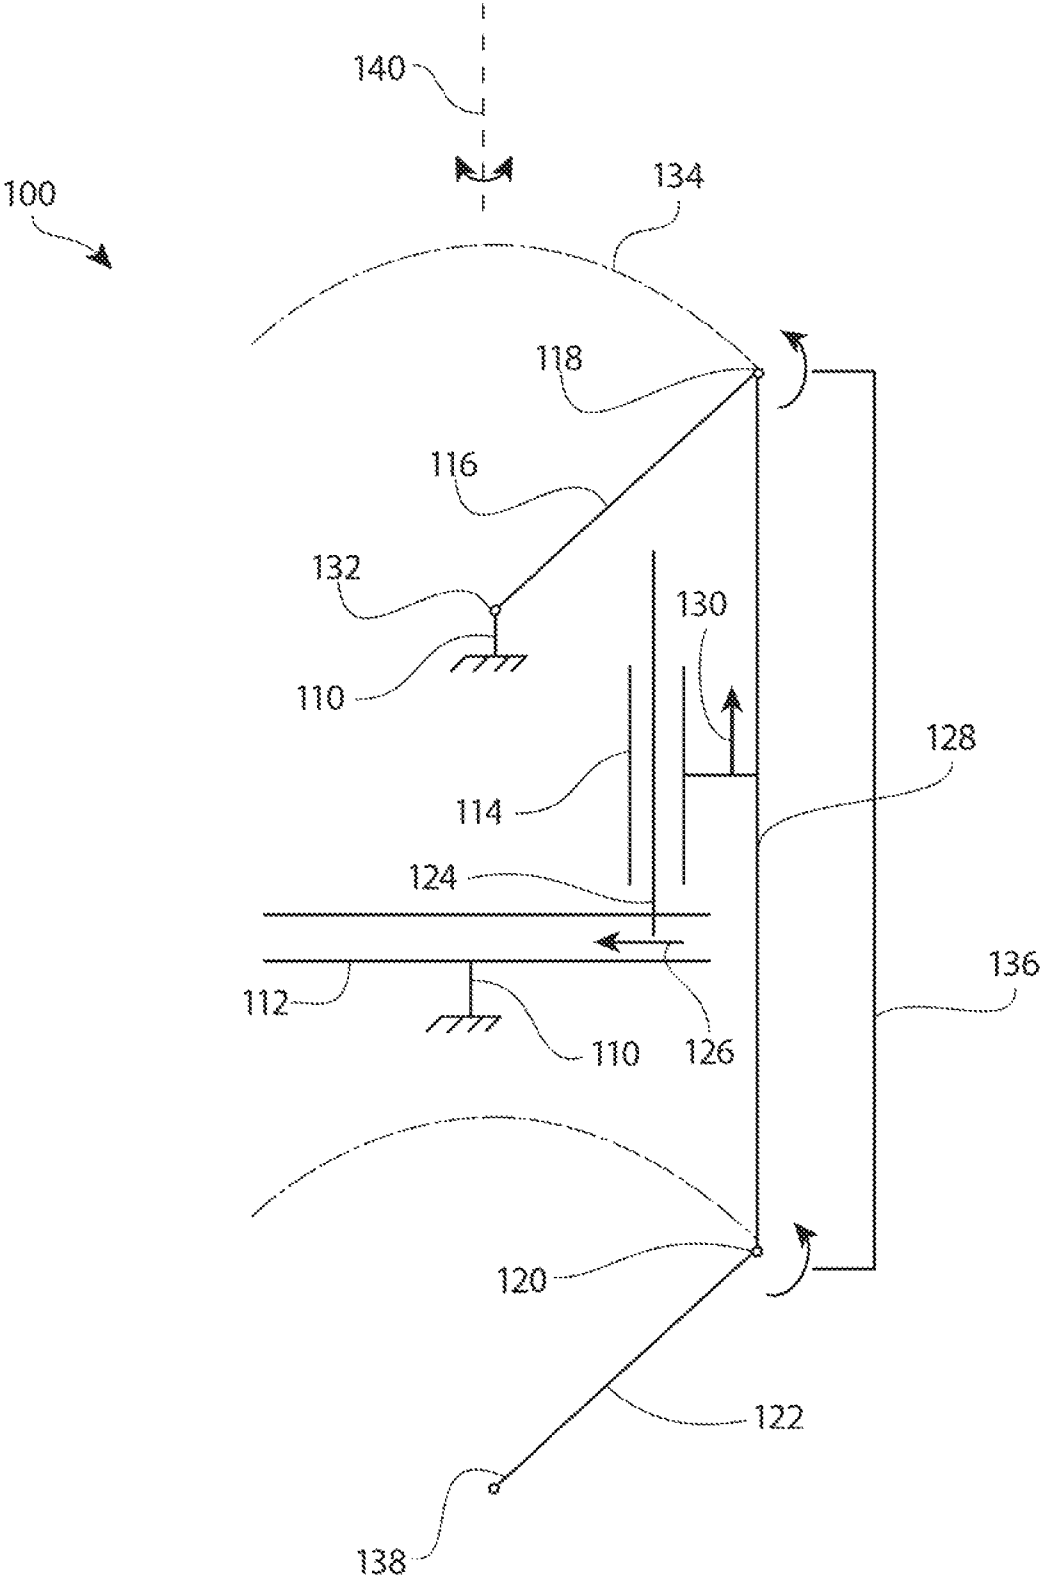


FIG. 1

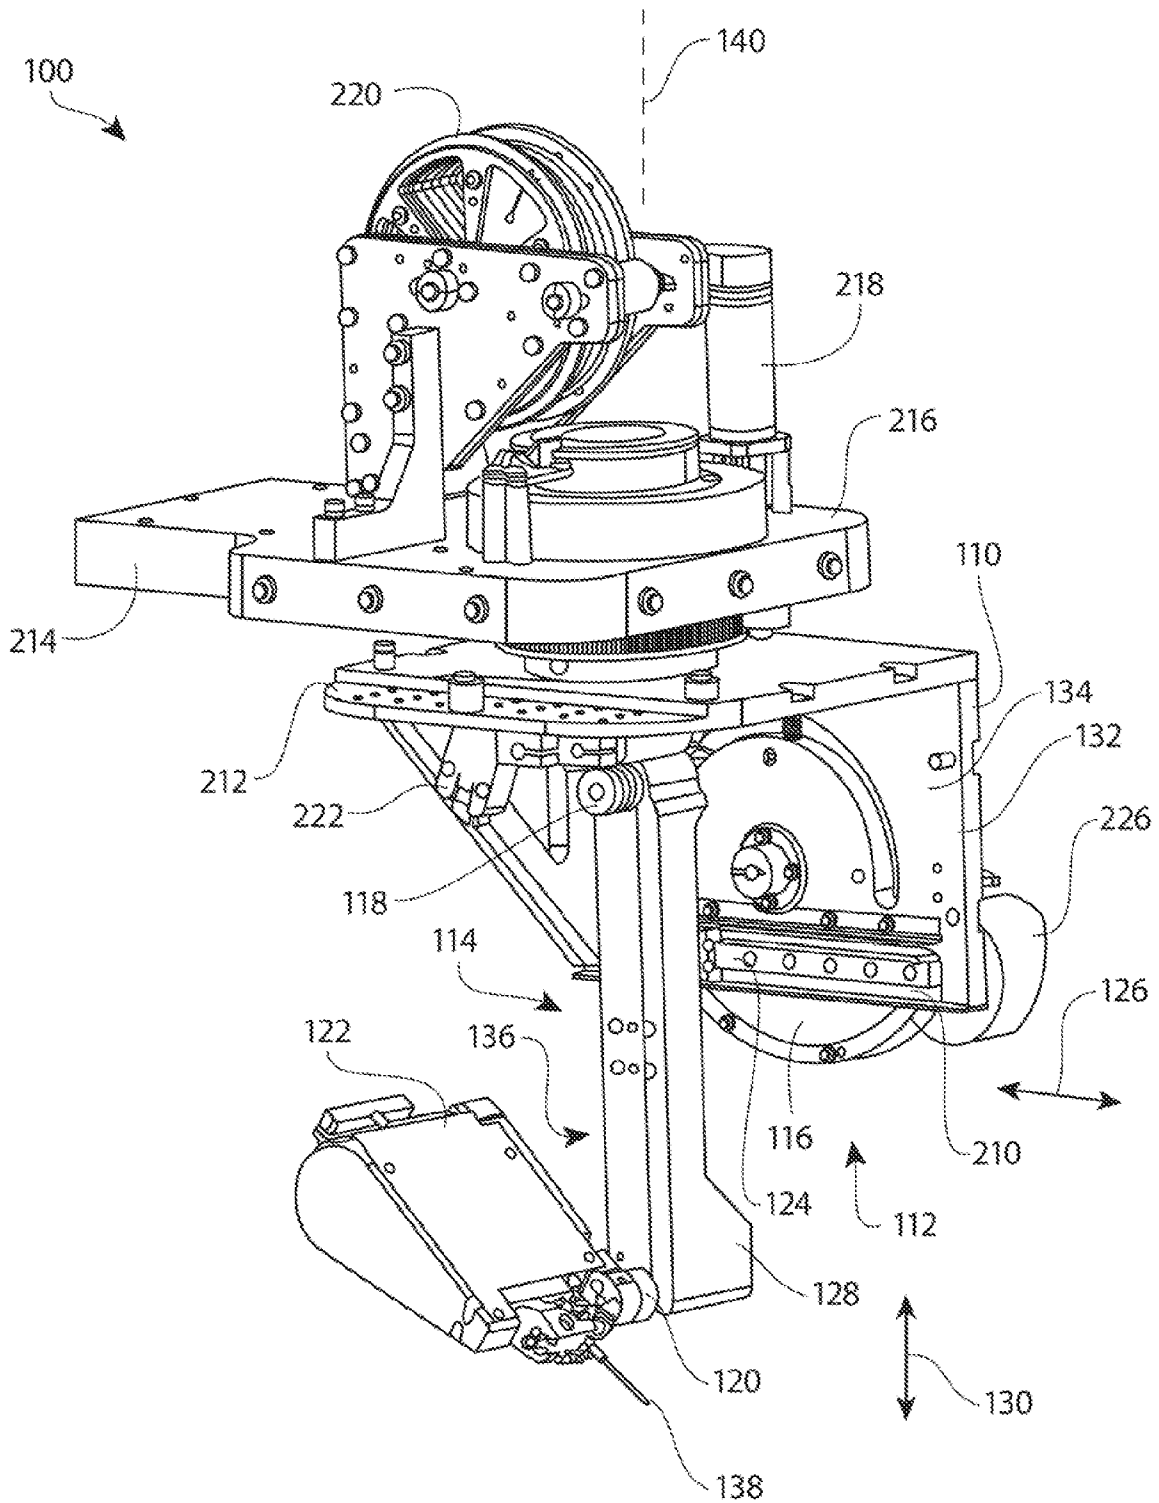


FIG. 2

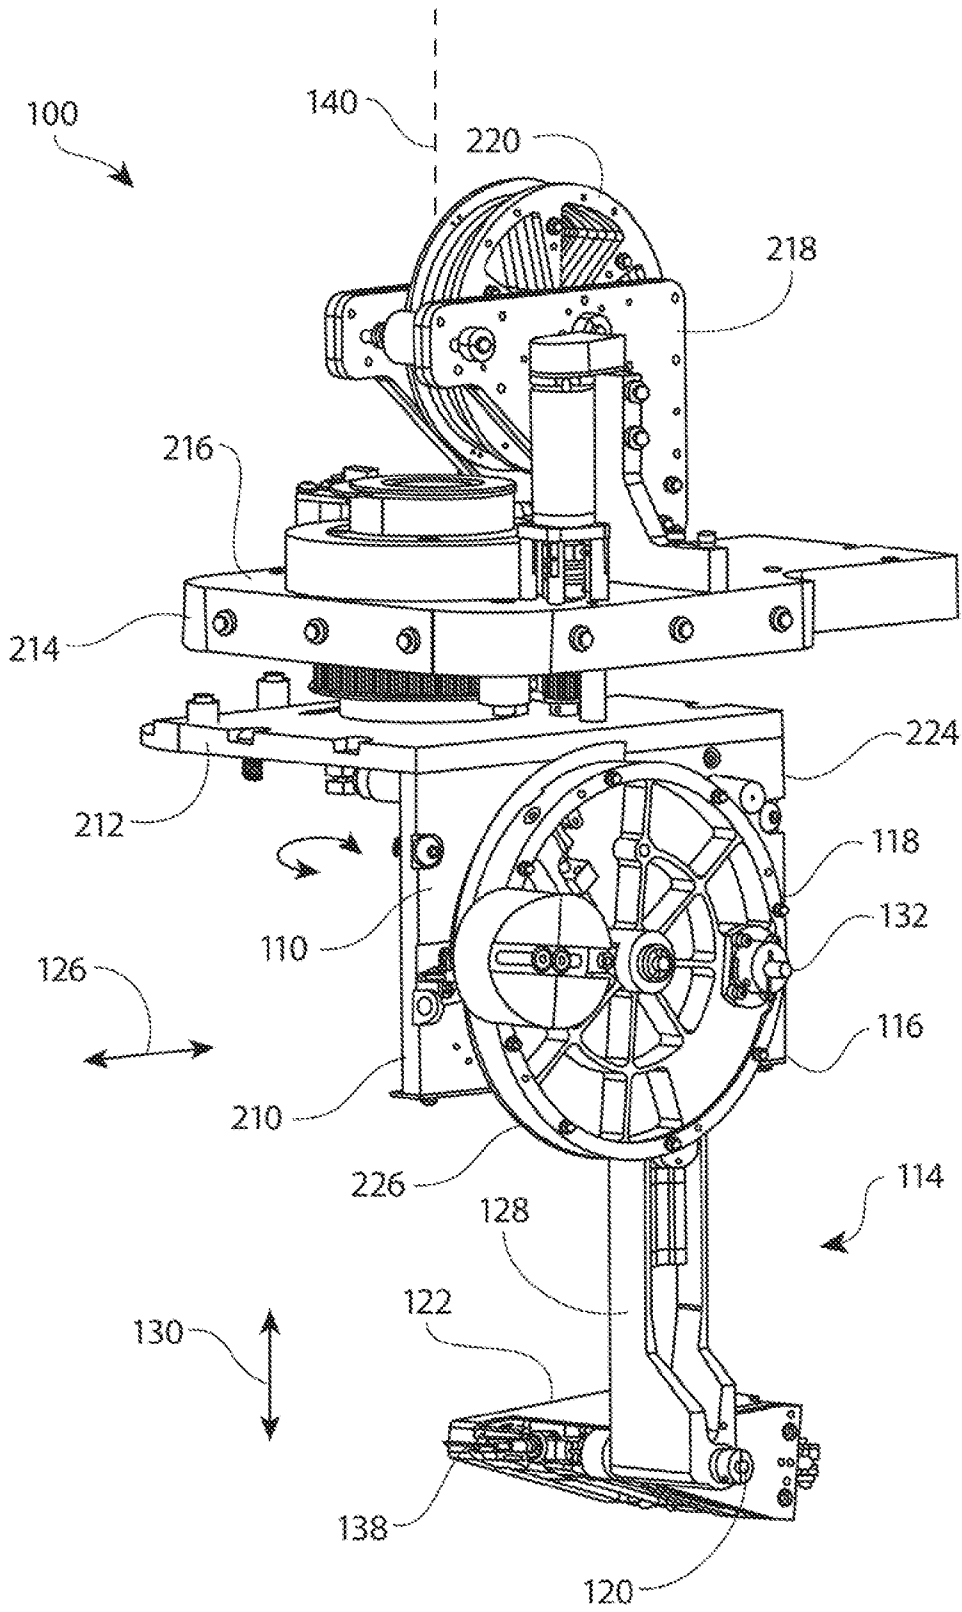


FIG. 3

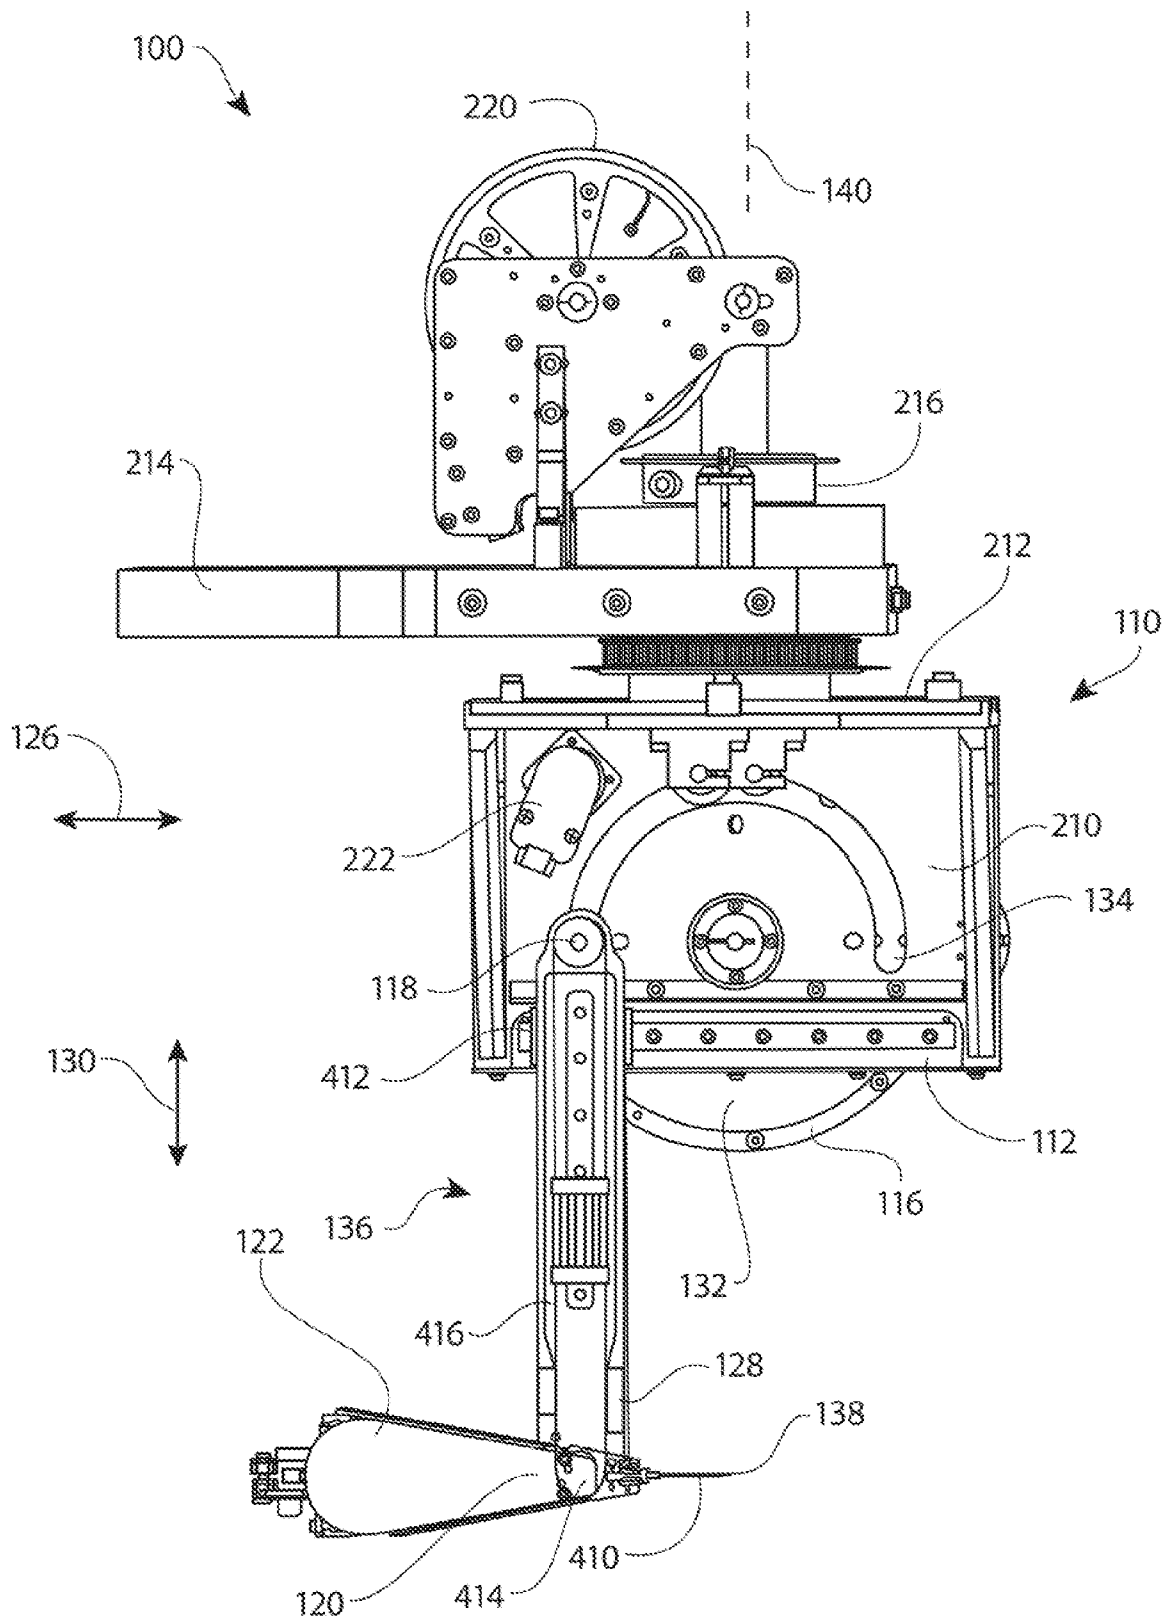


FIG. 4

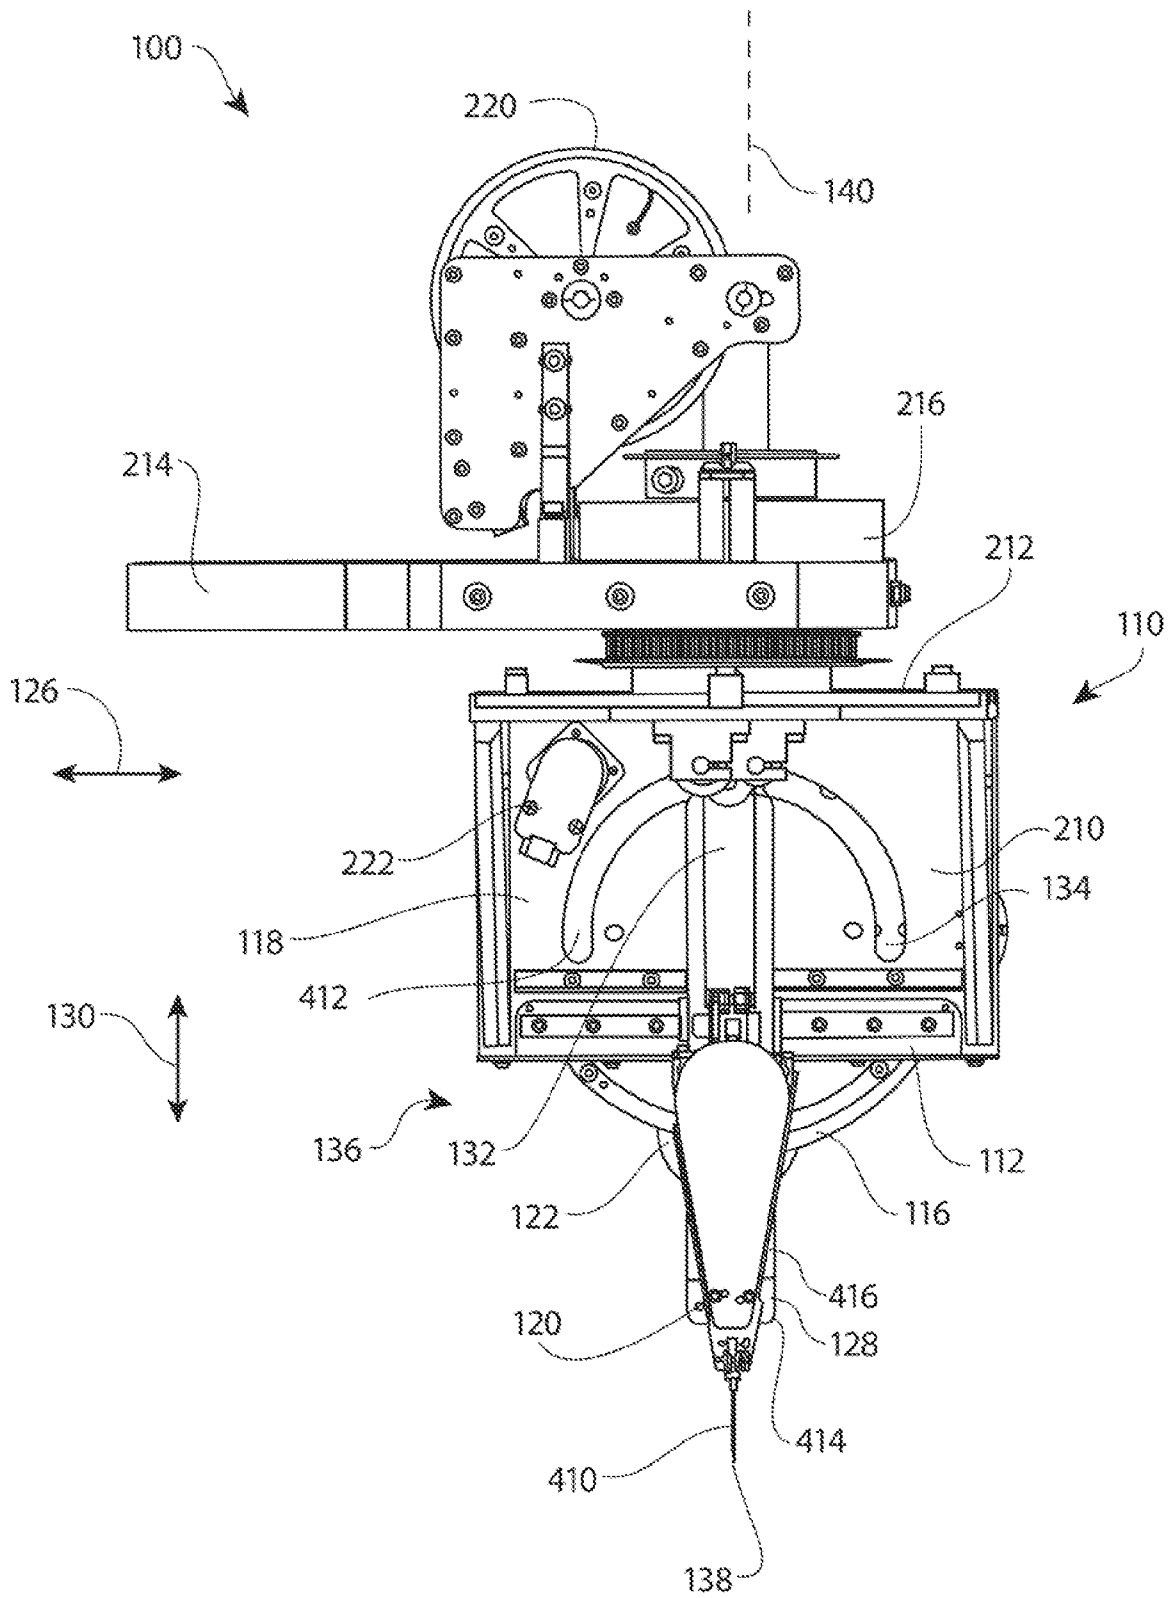


FIG. 5

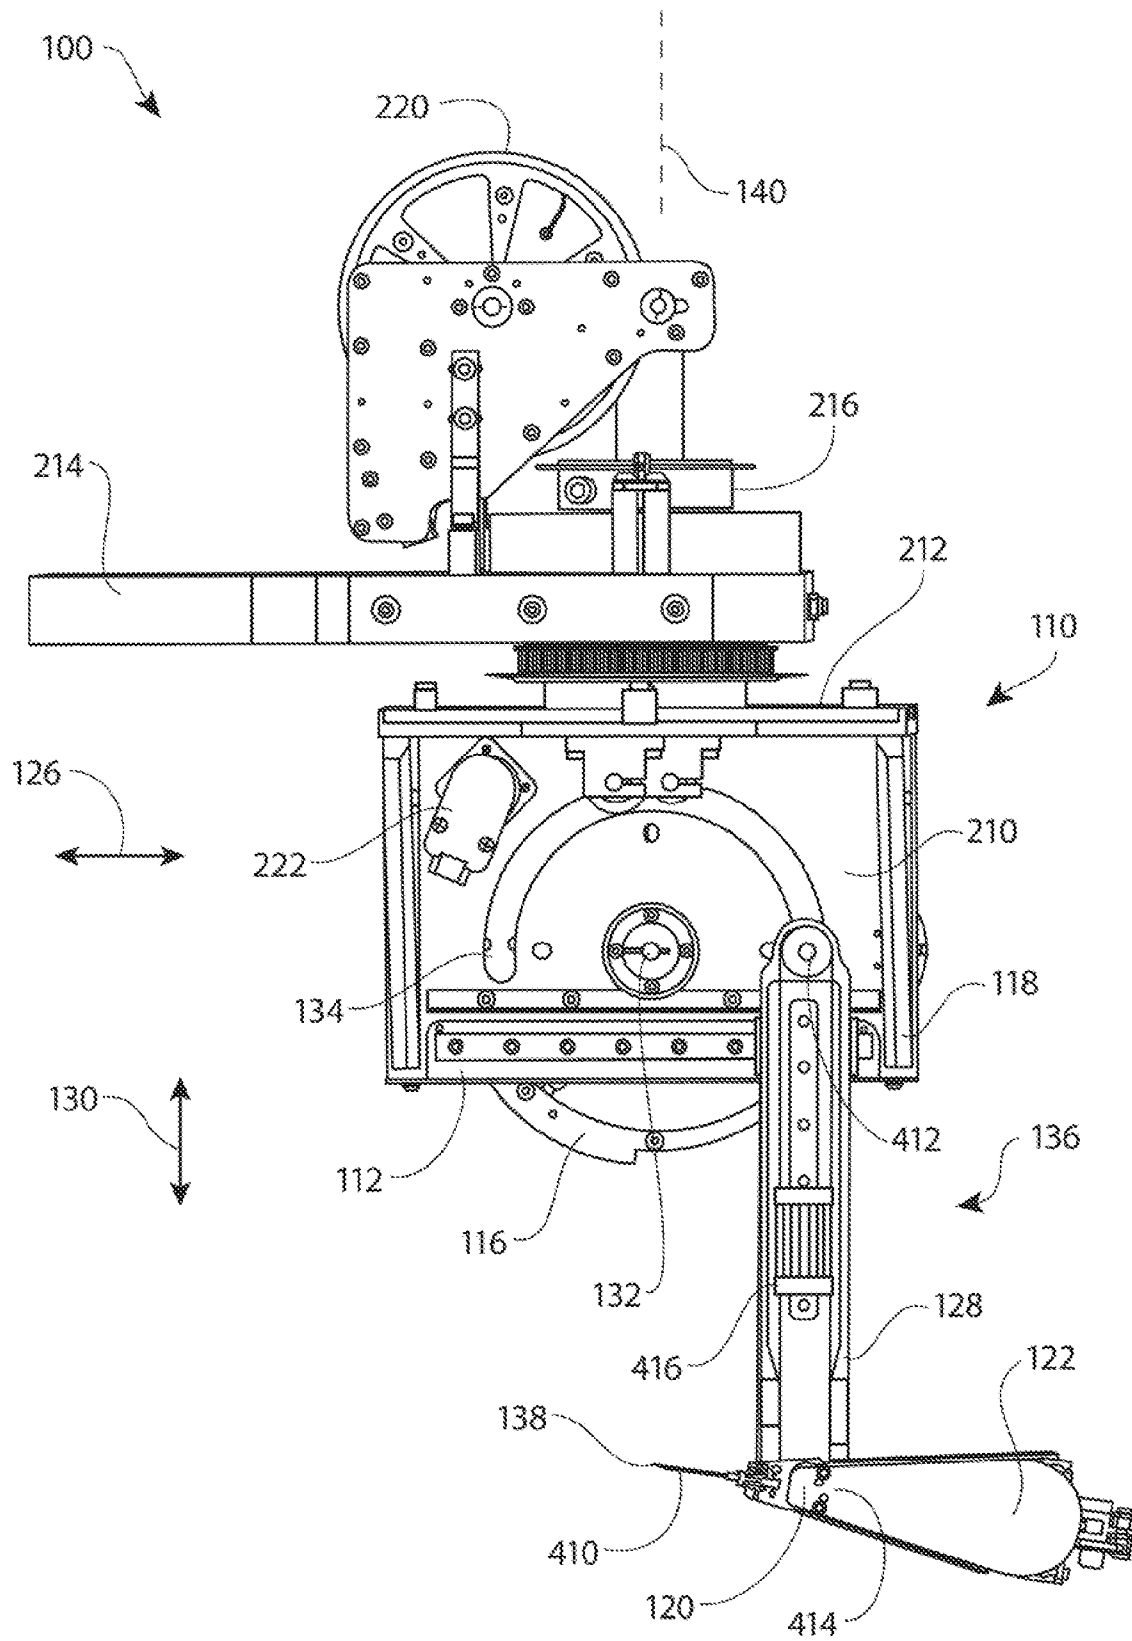


FIG. 6

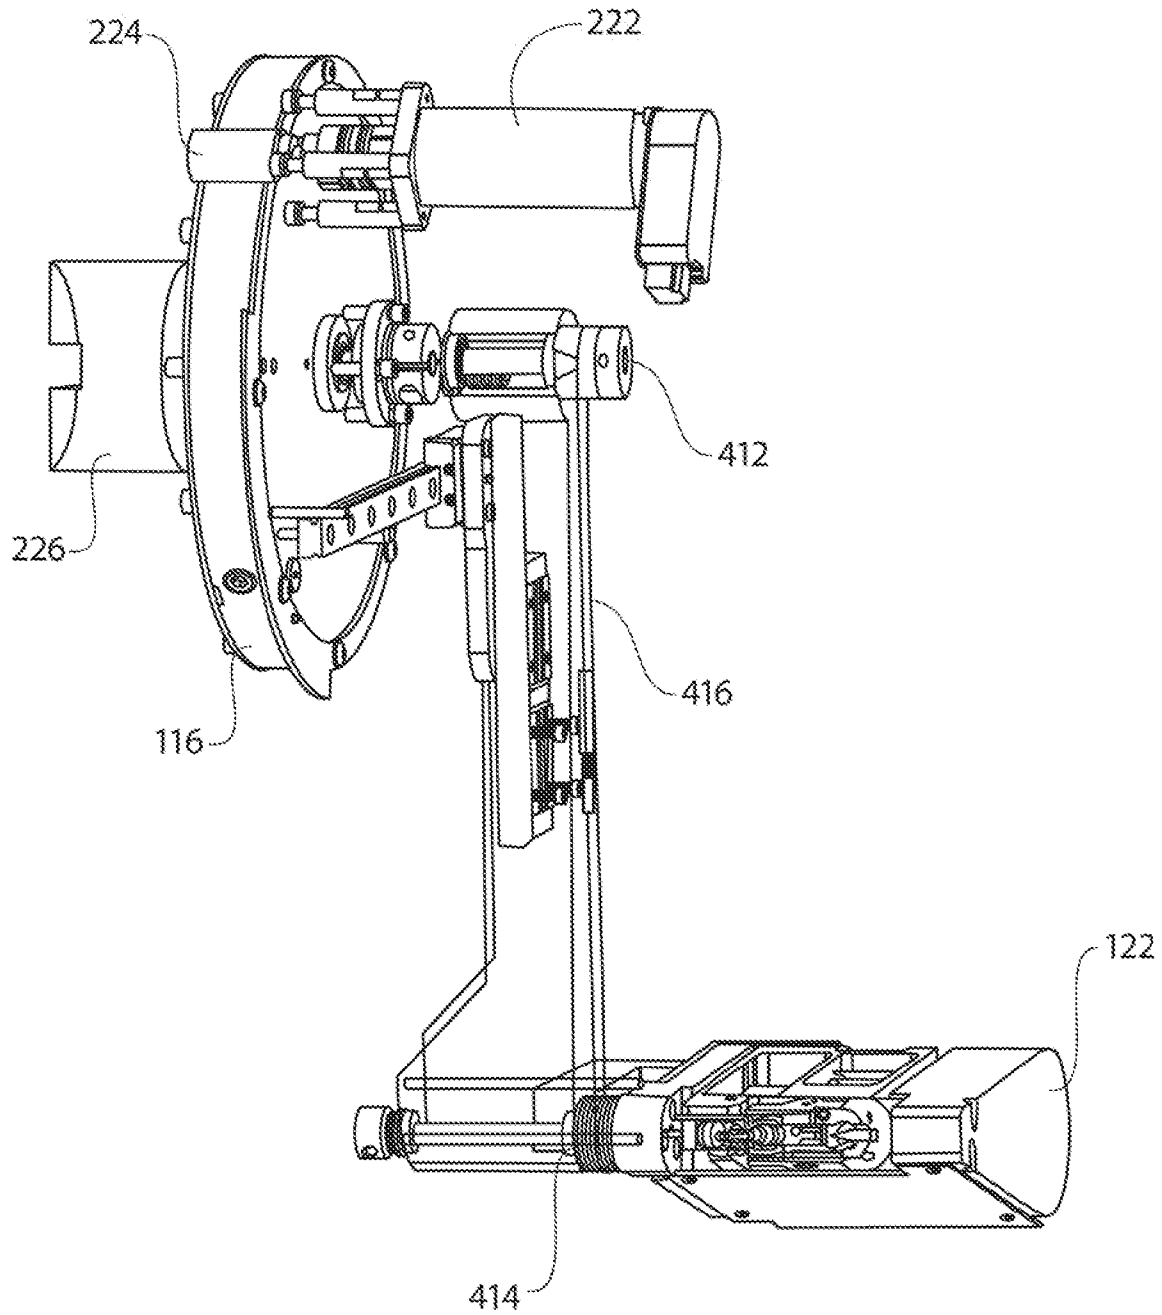


FIG. 7

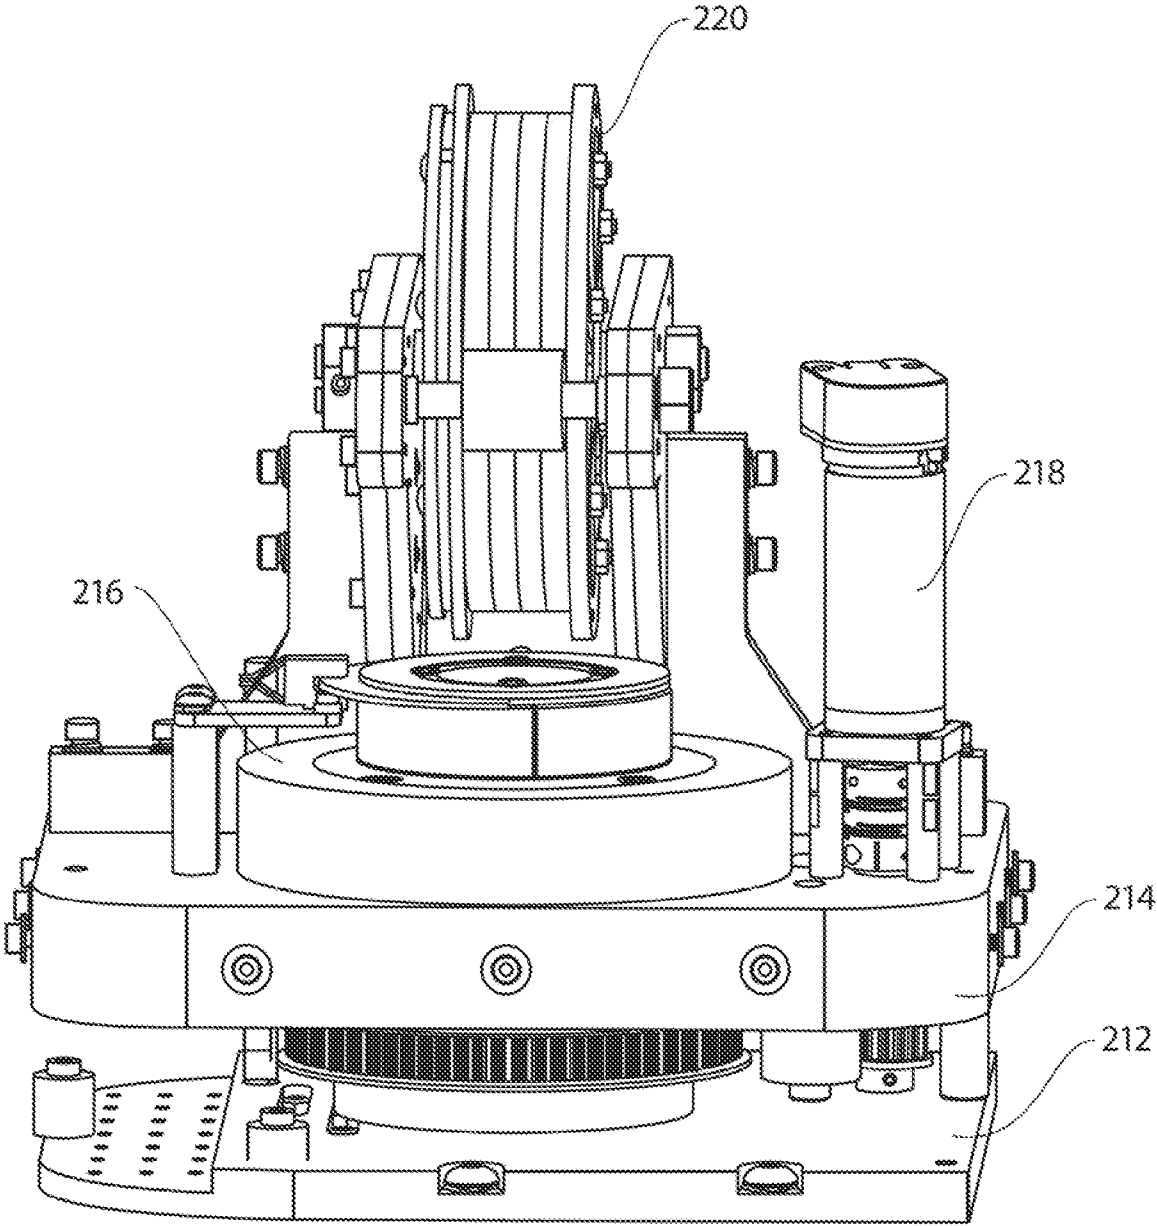


FIG. 8

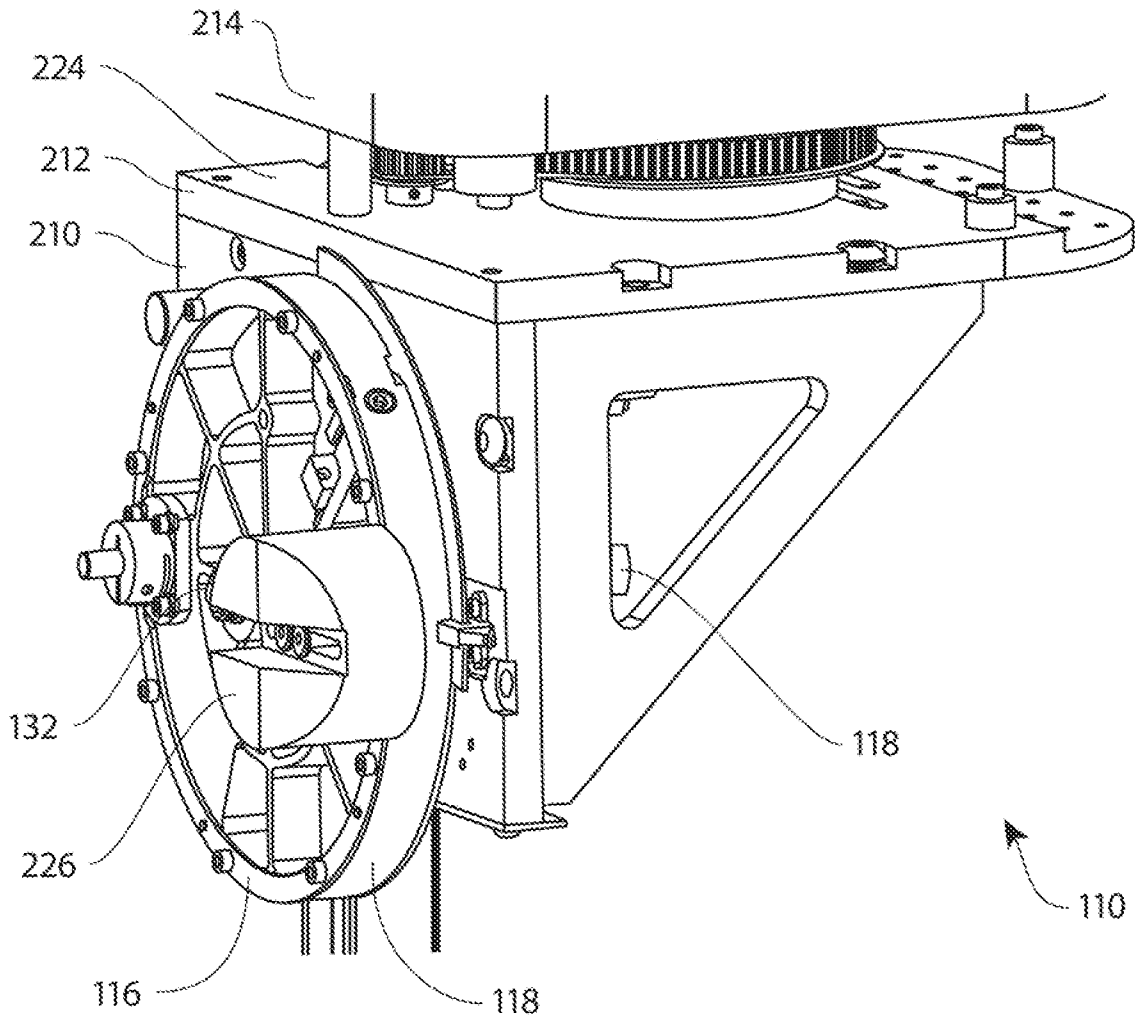


FIG. 9

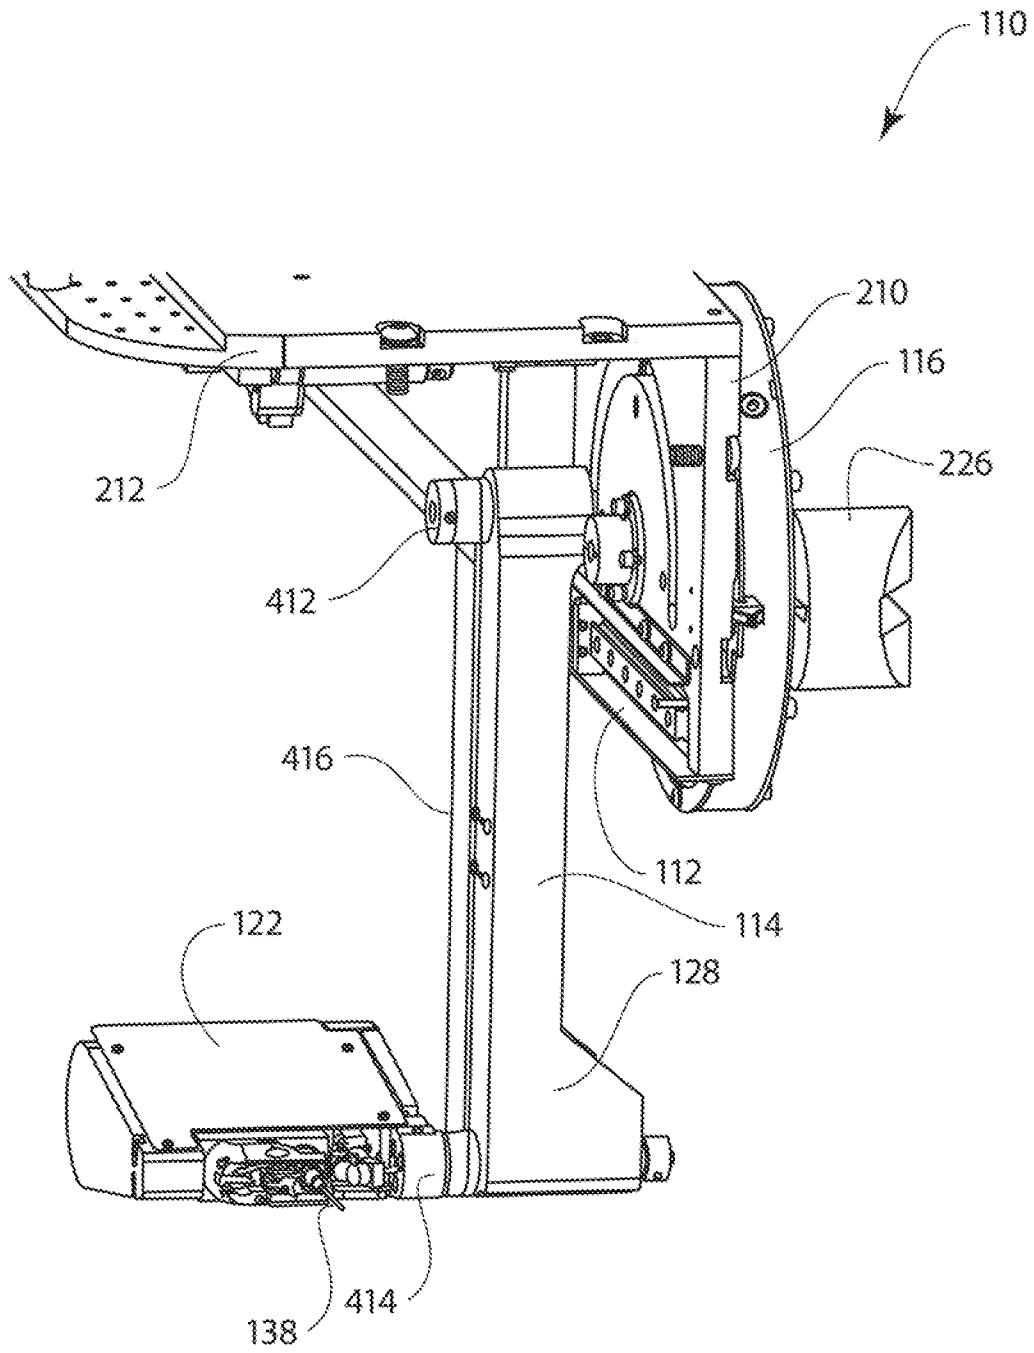


FIG. 10

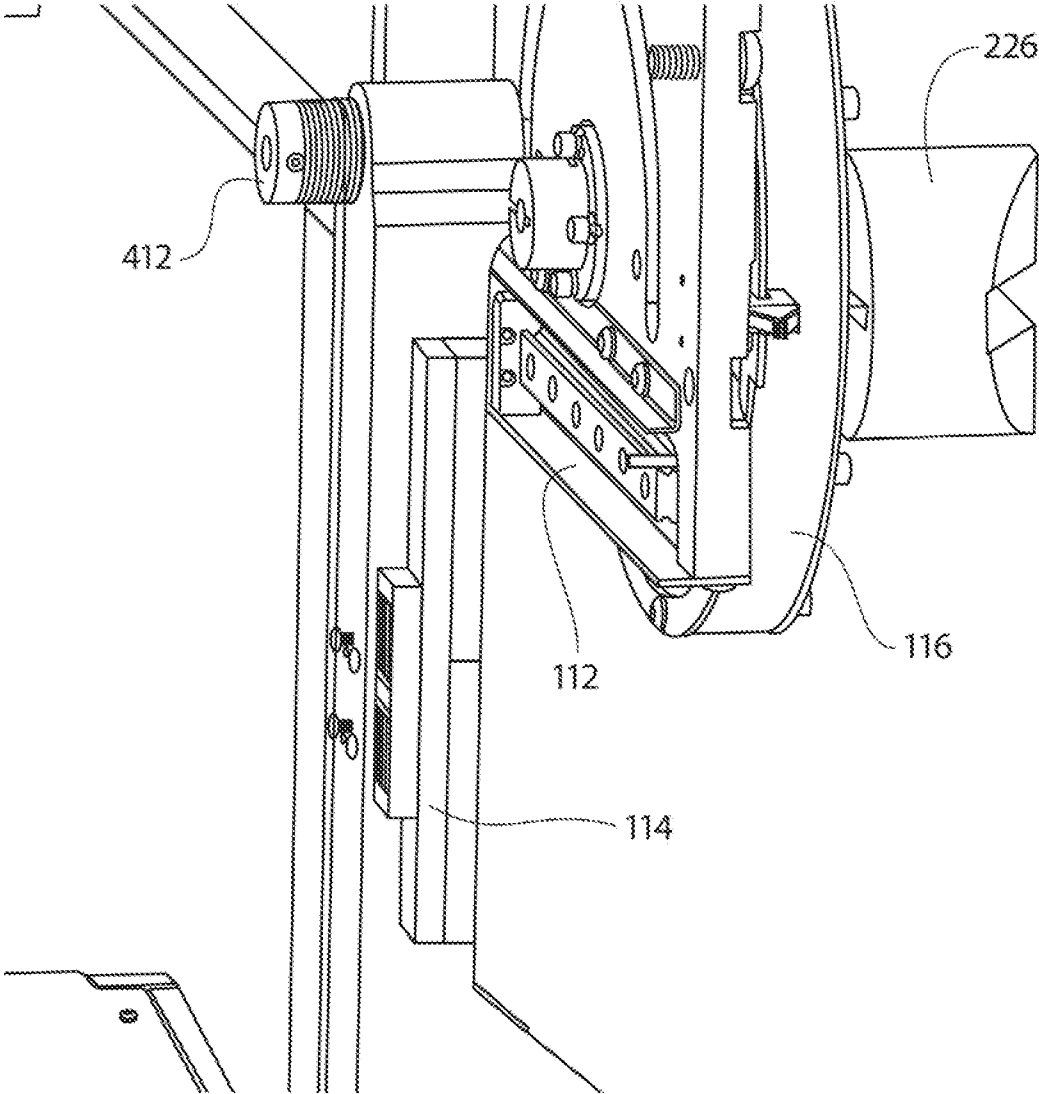


FIG. 11

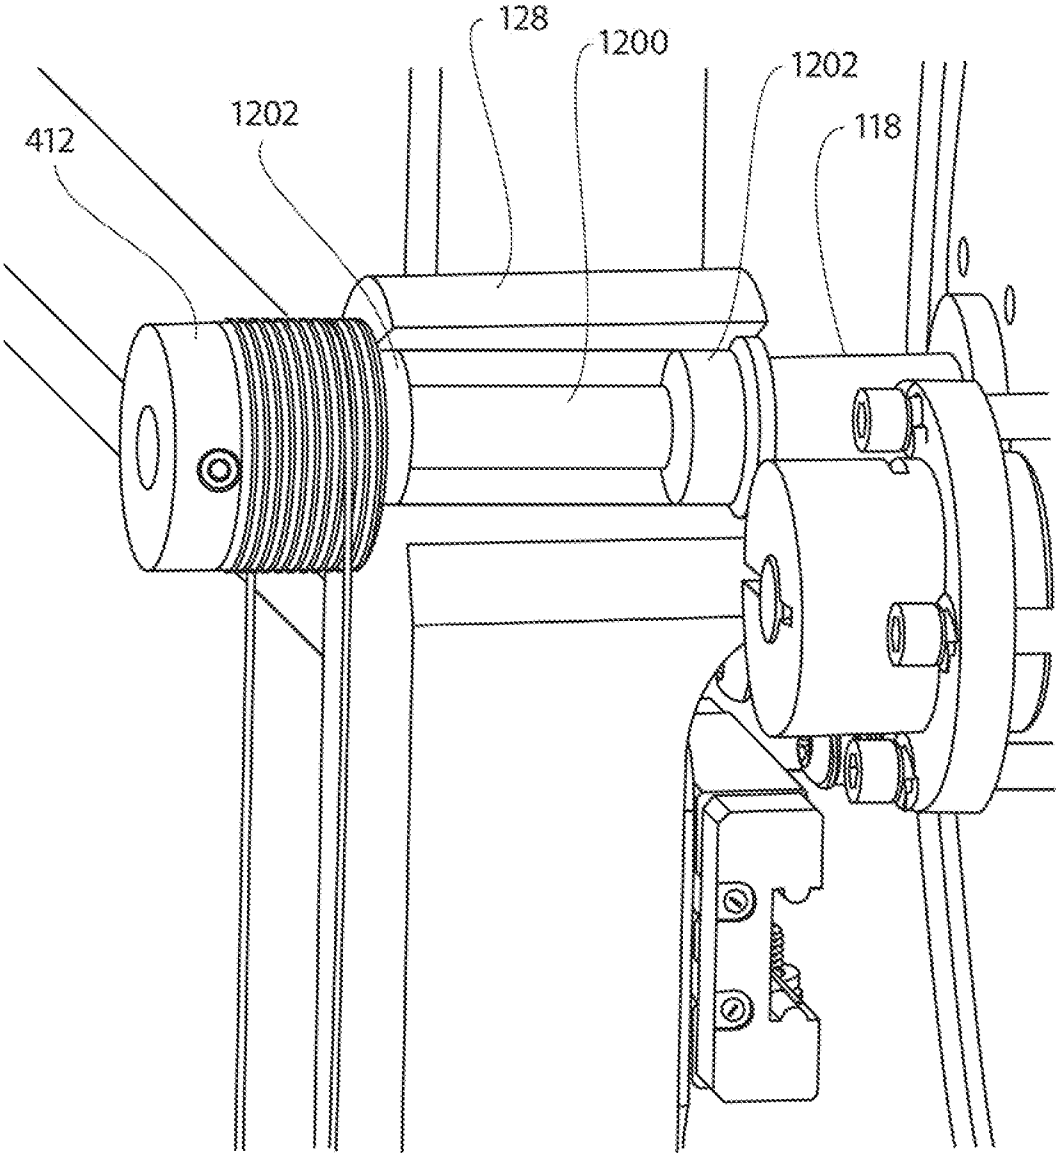


FIG. 12

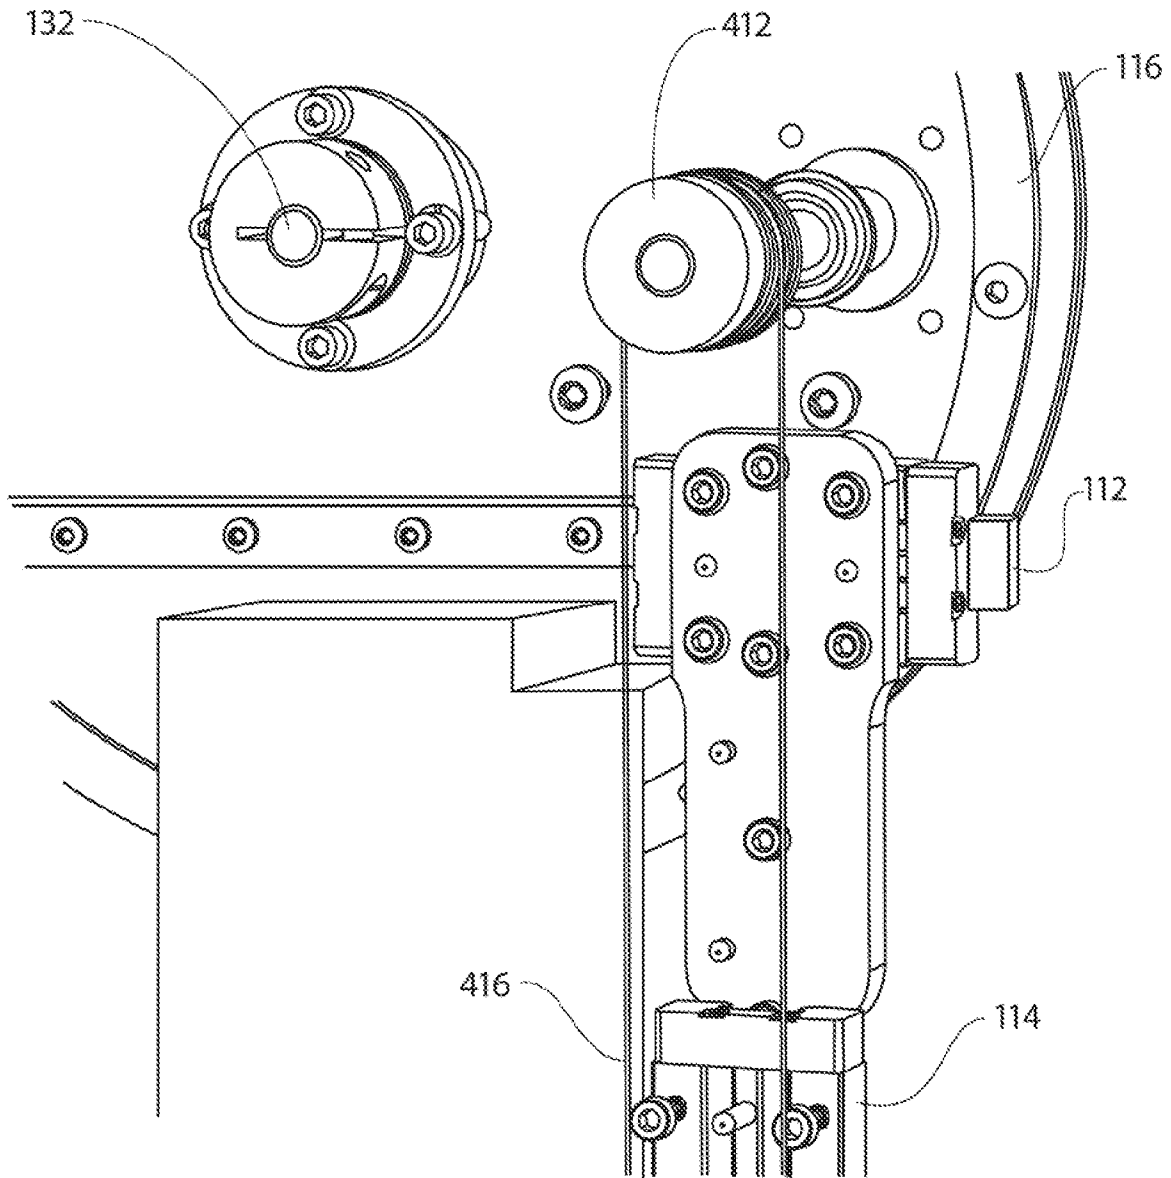


FIG. 13

REMOTE CENTER OF MOTION MECHANISM AND METHOD OF USE

CROSS REFERENCE TO RELATED APPLICATIONS

This patent application claims priority to provisional patent application Ser. No. 61/522,530, filed on Aug. 11, 2011 and titled "REMOTE CENTER OF MOTION MECHANISM AND METHOD OF USE."

INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

FIELD

The present invention relates generally to medical devices and, more particularly, to an apparatus for guiding a medical tool.

BACKGROUND

Apparatus for guiding medical tools have been shown to be of valuable assistance in various medical procedures, for example, manipulation of surgical tools, manipulation of cameras or sensors, biopsy, etc. An apparatus for guiding a medical tool usually also improves reproducibility compared to free-hand medical procedures, for example, surgical or biopsy procedures.

These apparatus typically have one or more degrees of freedom and may be manually driven in that the one or more degrees of freedom may be equipped with a brake with motive force being provided by a human practitioner, or may be automated in that at least one degree of freedom is driven by a computer controlled actuator.

A medical tool often needs to be oriented about a point in, on, or in proximity to a patient's body. However, having the main body of an apparatus that supports the tool located too proximal to the patient's body may be disadvantageous, since the supporting apparatus may, for example, interfere with the view of or access to the patient by the practitioner. An apparatus which can orient a tool about a remote fulcrum or remote center of motion can avoid such disadvantages.

The use of an apparatus that orients a tool about a remote center of motion is known in robotics as described, for example, in U.S. Pat. Nos. 5,397,323; 5,515,478; 5,630,431; 5,817,084; 5,907,664; 6,047,610; 6,246,200; and 7,021,173.

U.S. Pat. No. 5,397,323 to Taylor et al. discloses the remote center of motion principle in surgical robots with a first axis of rotation pointing into the remote center of motion, and a second axis materialized by a parallelogram mechanism implemented by two coupled parallel linkages of rigid bars and cylindrical joints. The two axes of the remote center of motion are orthogonal, and the mechanism operated around an upright initial (zero) direction.

Unfortunately, the parallelogram structure of Taylor et al. and other conventional parallelogram mechanisms is bulky, making it difficult to position with respect to a patient's body and in some cases forcing a patient to assume an uncomfortable or unconventional position. Therefore, there is a need for an alternative apparatus for guiding medical tools.

U.S. Pat. No. 5,817,084 discloses another exemplary linkage that provides a remote center of motion. The disclosed linkage arrangement allows the motors for positioning the insertion axis to be at a distance from the center of motion. However, the first motor is required to move the entire mass of the second motor in the disclosed linkage arrangement. This requires a larger first motor. The second motor sweeps out a volume as it is moved. Both of these shortcomings increase the mass and bulk of the disclosed linkage arrangement.

In certain applications it is desirable to provide a robotic manipulator device having an end effector that can pass through a small opening in a wall. One way this can be done is to introduce the end effector along an insertion axis with the axis constrained to rotate about a point substantially at the point where the insertion axis intersects the wall, which may be termed the center of motion for the insertion axis.

It will be appreciated that the position of the end effector can be expressed in a spherical coordinate system with an origin at the center of motion. The end effector position may be expressed as two angular displacements and a radius, which is the distance from the center of motion to the end effector. Thus the end effector can be positioned at any point within the range of motion of the robotic manipulator while passing through a small opening in a wall.

One application of such a robotic manipulator is the positioning of an end effector for performing surgical procedures. Minimally invasive surgery (MIS) provides surgical techniques for operating on a patient through small incisions using a camera and elongate surgical instruments introduced to an internal surgical site, often through trocar sleeves or cannulas. The surgical site often comprises a body cavity, such as the patient's abdomen. The body cavity may optionally be distended using a clear fluid such as an insufflation gas. In robotic minimally invasive surgery, the surgeon manipulates the tissues using end effectors of the elongate surgical instruments by remotely manipulating the instruments while viewing the surgical site on a video monitor. As previously mentioned, it may be impractical to place the motors for positioning the insertion axis in proximity to the center of motion. The robotic manipulator may include linkages to couple the motors for positioning the insertion axis at a distance from the center of motion.

The manipulator devices and methods disclosed herein provide advantages over those of the prior art.

SUMMARY OF THE DISCLOSURE

According to one exemplary embodiment, a manipulator device includes a base, first and second linear slides, a drive link, a drive member, a driven member and an end effector. The first linear slide is mounted to the base and has a first carriage movable along a first axis. The second linear slide is mounted to the first carriage and has a second carriage movable along a second axis orthogonal to the first axis. The drive link is coupled between the base and the second carriage and is rotatable about a proximal center of motion that is fixed relative to the base. The drive link is configured to move the second carriage in a constant radius arcuate path relative to the base. The first and second linear slides constrain the second carriage to have a non-rotating orientation relative to the base as the second carriage moves along the arcuate path. The drive member is carried by the second carriage and is connected to the drive link such that the drive member rotates with respect to the second carriage as it moves along the arcuate path but maintains the same rotational orientation as the drive link. The driven member is also carried by the second carriage. The driven member is laterally spaced apart

3

from and rotationally coupled to the drive member such that the driven member rotates with respect to the second carriage as it moves along the arcuate path but maintains the same rotational orientation as the drive member and the drive link. The end effector is carried by the second carriage and is rotationally coupled to the driven member such that the end effector maintains the same rotational orientation as the driven member, the drive member, and the drive link. The elements of the manipulator device cooperate to constrain the end effector to rotate about a remote center of motion that is displaced from the proximal center of motion as the drive link moves the second carriage along the arcuate path.

In some embodiments, the base is rotatable about an axis that intersects the proximal center of motion and the remote center of motion such that the end effector is spherically rotatable in two degrees of freedom about the remote center of motion.

In some embodiments, the manipulator device comprises a prime mover coupled to the drive link and configured to move the second carriage along the arcuate path. The device may include an automated mode in which at least one degree of freedom is driven by a computer controlled actuator. In some embodiments, the end effector is configured to be manually moved, and the drive link is configured to follow the motion of the second carriage and constrain the second carriage to move along the arcuate path. The manipulator device may include a powered assist mode in which manual movements of the end effector are sensed and a prime mover provides force to assist with those movements. The device may include a manual mode and a powered assist mode as previously described, and an automated mode in which at least one degree of freedom is driven by a computer controlled actuator.

In some embodiments of the manipulator device, the end effector comprises an intravenous line inserter. In some embodiments, the device comprises shaft encoders to provide feedback of rotational positions in the two degrees of freedom about the remote center of motion.

Methods of using the above manipulator devices are also disclosed.

Areas of use for the methods and devices disclosed herein include, for example, laparoscopic surgery, intravenous line insertion, and stapedectomy (ear surgery), each with or without robotic assistance.

Other features and advantages of the present invention will be apparent from the accompanying drawings and from the detailed description that follows below.

BRIEF DESCRIPTION OF THE DRAWINGS

A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, and the accompanying drawings of which:

FIG. 1 is a schematic representation of an exemplary remote center of motion device constructed according to aspects of the disclosure;

FIGS. 2 and 3 are perspective views showing further details of the device of FIG. 1;

FIGS. 4-6 are a series of front elevation views showing the device of FIG. 1 in a progression of positions;

FIG. 7 is a side elevation view showing a lower portion of the device of FIG. 1;

FIG. 8 is a perspective view showing an upper portion of the device of FIG. 1;

FIG. 9 is an oblique side elevation view showing a rear portion of the device of FIG. 1;

4

FIG. 10 is an oblique side elevation view showing a front portion of the device of FIG. 1;

FIG. 11 is an enlarged view showing a portion of FIG. 10;

FIG. 12 is a further enlarged view showing a portion of FIG. 11;

FIG. 13 is an enlarged frontal view showing a calibration tool being used with the exemplary device of FIG. 1.

DETAILED DESCRIPTION

Referring to FIG. 1, an exemplary manipulator system constructed according to aspects of the disclosure is schematically shown. In this exemplary embodiment, a manipulator device 100 includes a base 110, first and second linear slides 112 and 114, a drive link 116, a drive member 118, a driven member 120 and an end effector 122. The first linear slide 112 is mounted to the base 110 and has a first carriage 124 movable along a first axis 126. The second linear slide 114 is mounted to the first carriage 124 and has a second carriage 128 movable along a second axis 130 orthogonal to the first axis 126. The drive link 116 is coupled between the base 110 and the second carriage 128 and is rotatable about a proximal center of motion 132 that is fixed relative to the base 110. The drive link 116 is configured to move the second carriage 128 in a constant radius arcuate path 134 relative to the base 110. The first and second linear slides 112 and 114 constrain the second carriage 128 to have a non-rotating orientation relative to the base 110 as the second carriage 128 moves along the arcuate path 134. The drive member 118 is carried by the second carriage 128 and is connected to the drive link 116 such that the drive member 118 rotates with respect to the second carriage 128 as it moves along the arcuate path 134 but maintains the same rotational orientation as the drive link 116. The driven member 120 is also carried by the second carriage 128. The driven member 120 is laterally spaced apart from and rotationally coupled to the drive member 118 by a coupling rotational coupling device 136 such that the driven member 120 rotates with respect to the second carriage 128 as it moves along the arcuate path 134 but maintains the same rotational orientation as the drive member 118 and the drive link 116. The end effector 122 is carried by the second carriage 128 and is rotationally coupled to the driven member 120 such that the end effector 122 maintains the same rotational orientation as the driven member 120, the drive member 118, and the drive link 116. The elements of the manipulator device 100 cooperate to constrain the end effector 122 to rotate about a remote center of motion 138 (which may also be referred to as a pitch axis) that is displaced from the proximal center of motion 132 as the drive link 116 moves the second carriage 128 along the arcuate path 134. Thus, in some embodiments, the final desired motion provided by manipulator device 100 is that end effector 122 rotates in a circle, with the tip of end effector 122 always at the center of the circle and the body of end effector 122 always oriented along a radius of the circle.

In some embodiments, the base 110 carrying all of the previously described components is rotatable about a yaw axis 140 that intersects the proximal center of motion axis 132 and the remote center of motion axis 138. With this added degree of freedom, the end effector 122 becomes spherically rotatable in two degrees of freedom about the remote center of motion 138. Thus, in some embodiments, the final desired motion provided by manipulator device 100 is that end effector 122 rotates within a sphere, with the tip of end effector 122 always at the center of the sphere and the body of end effector 122 always oriented along a radius of the sphere.

In some embodiments, the manipulator device **100** further comprises a prime mover (not shown in FIG. **1**) coupled to the drive link **116** and configured to move the second carriage **128** along the arcuate path **134**. In some embodiments, the end effector **122** of the manipulator device **100** is configured to be manually moved, and the drive link **116** is configured to follow the motion of the second carriage **128**. In other words, the drive link **116** and drive member **118** do not actually “drive” the second carriage **128** and the driven member **120**, but serve merely to constrain the second carriage **128** to move along the arcuate path **134** and maintain a desired orientation of the end effector **122**. In some embodiments, the manipulator device has both an automatically driven mode and a manually operated mode. In some embodiments, the manipulator device has a powered assist mode, in which manual movements of the end effector **122** are sensed and a prime mover provides force to assist with those movements, such as assisting with acceleration, deceleration, and/or maintaining a sensed velocity and/or position. Shaft encoders may be provided as shown to provide feedback of the rotational positions of the pitch and yaw axes.

Referring to FIGS. **3** and **4**, further details of exemplary manipulator device **100** are shown. In this exemplary embodiment, base **110** comprises a vertical plate **210** and a horizontal plate **212** attached together in an L-shaped arrangement. Base **110** is rotatably mounted to frame **214** with bearing **216** such that base **110** may be rotated relative to frame **214** about vertical yaw axis **140**. A motor **218** may be attached to frame **214** for rotating base **110** through a timing belt pulley and belt system as shown. Frame **214** may be fixed relative to ground, or may add further degrees of freedom by being movably mounted, such as by being vertically adjustable. A constant tension cable spool **220** may be provided atop frame **214** for taking up slack in wires, cables, tubing, etc. (not shown), which may pass from spool **220** through a central aperture in bearing **216** along vertical yaw axis **140** to the pivoting end effector **122**.

In this exemplary embodiment, drive link **116** is formed by a wheel mounted with bearings to rotate about the proximal center of motion axis **132**. A motor **222** (shown in FIG. **2**) may be provided on a front side of base plate **210** for rotatably driving drive link **116** with a capstan **224** (shown in FIGS. **3** and **7**) provided on a backside of base plate **210**. Capstan **224** drives the outer circumference of drive link wheel **116** to rotate it, such as with a cable transmission having a cable that is wound around capstan **224** and wheel **116**.

As best seen in FIG. **3**, drive member **118** may comprise a shaft rigidly mounted to drive link wheel **116**. As best seen in FIG. **2**, drive member **118** passes through a slot in base plate **210** which forms arcuate path **134**. In this embodiment, drive member **118** may travel about 190 degrees along arcuate path **134**. In other embodiments, different ranges of motion may be provided, such as about 45, 90, 180, 270, 350, 360, 450 degrees, or infinite travel. For embodiments having travel greater than about 350 degrees, drive link/wheel **116** or a portion thereof may be mounted on the same side of vertical base plate **210** as slides **112** and **114** so that drive member **118** need not pass through a slot **134** in plate **210**. The distal end of drive member **118** may pass through second carriage **128** as shown and may include a cable pulley mounted thereon, as will subsequently be described in further detail. Referring again to FIG. **3**, drive link wheel **116** may be provided with a weight **226** opposite from drive member **118** to counterbalance the weight of second slide **114** and end effector **122**.

Referring again to FIG. **2**, it can be seen that first slide **112** is rigidly mounted to base plate **210**, allowing first carriage **124** to travel back and forth horizontally with respect to base

plate **210**. Second slide **114** is rigidly mounted to first carriage **124**, allowing second carriage **128** to travel back and forth vertically with respect to first carriage **124**. With this arrangement, driving drive link wheel **116** with motor **222** causes second carriage **128** to travel along arcuate path **134**. During this travel, the vertical orientation of second carriage **128** is maintained by virtue of its coupling to base plate **210** through first and second linear slides **112** and **114**.

Referring to FIGS. **4-6**, the rotation of end effector **122** about the remote center of motion **138** will now be described. It can be seen from the progression of FIGS. **4-6** that as second carriage **128** and end effector **122** travel together along arcuate path **134** from roughly the 9 o'clock position (FIG. **4**), through the 12 o'clock position (FIG. **5**) to roughly the 3 o'clock position (FIG. **6**), end effector **122** changes orientation from pointing roughly 90 degrees to the right (FIG. **4**), to pointing straight down (FIG. **5**), to pointing roughly 90 degrees to the left (FIG. **6**). In this exemplary embodiment, end effector **122** may be an intravenous line inserter. If needle **410** of end effector **122** is arranged so that its distal tip is spaced apart from the axis of rotation of driven member **120** by a distance equal to the spacing between the axis of rotation of drive member **118** and the proximal center of motion **132**, the distal tip of needle **410** will always be on the remote center of motion **138** regardless of its pivoting orientation, and the orientation of needle **410** will always be along a radius of a circle having its center on the remote center of motion **138**.

The above-described pivoting of needle **410** about the remote center of motion **138** is accomplished by rotational coupling device **136**, which may include a first pulley **412** rigidly attached to the distal end of drive member **118**, a second pulley **414** rigidly attached to the distal end of driven member **120**, and a drive cable **416** interconnecting the first and second pulleys. Drive member **118** and driven member **120** may each comprise a shaft **1200** rotatably supported by second carriage **128**, such as with bushings or with ball bearings **1202**, as best seen in FIG. **12**. With this arrangement, first pulley **412** and second pulley **414** rotate in unison relative to second carriage **128**. Since drive member **118** is rigidly connected to drive link wheel **116**, it can be appreciated that the orientation of first pulley **412** will rotate 180 degrees clockwise as it travels along arcuate path **134** from the 9 o'clock position shown in FIG. **4** to the 3 o'clock position in FIG. **6**. During this motion, second pulley **414** will also rotate 180 degrees clockwise since it is rotationally coupled to first pulley **412** by cable **416**. Second pulley **414** in turn rotates end effector **122** the same amount.

Further details of exemplary manipulator device **100** are shown in FIGS. **7-13**. According to aspects of the disclosure, manipulator device **100** is configured to pass through a vertical inflection point, as depicted in FIGS. **4-6**. Device **100** is easy to calibrate, is more compact, and includes fewer moving parts, cables and potential pinch points than prior art remote center of motion manipulators.

As with many robotic manipulators that support and position an end effector with a remote center of motion, manipulator **100** comprises a cantilevered structure. As previously described, manipulator **100** is supported from an end of the structure opposite the end that supports the end effector. In some embodiments it is desirable that the manipulator be stiff so that the position of the end effector can be controlled with great precision. Stiffness may generally be achieved by providing a structure with a high resonant frequency and a low moment of inertia. Thus it is often desirable to minimize the mass of the manipulator and the distance of the mass from the supported end of the cantilevered structure. The arrangement

7

of manipulator **100** advantageously places the motors and other components having a large mass in a compact configuration that minimizes the contribution of these relatively heavy components to the moment of inertia of the manipulator.

In this or other embodiments, either side of a linear slide can be considered a “carriage”. In some embodiments, a drive member and a driven member can be a pair of pulleys, sprockets, capstans, gears, lever arms or servos, coupled by one or more cables, chains, belts, gear trains, tie rods, or conductors. Other suitable mechanisms may also be used to transfer rotational orientation between a drive member and a driven member. In some embodiments, a drive link may be a wheel, lever arm, cam groove or other suitable mechanism. A drive link and/or base can be rotated manually, or by one or more prime movers such as an electric motor. The electric motor(s) can be directly controlled by an operator, such as with a hand or foot-operated switch, or may be computer controlled with software.

While exemplary embodiments constructed according to aspects of the present invention have been shown and described herein, it will be obvious to those skilled in the art that such embodiments are provided by way of example only. Numerous variations, changes, and substitutions will now occur to those skilled in the art without departing from the invention. It should be understood that various alternatives to the embodiments of the invention described herein may be employed in practicing the invention.

What is claimed is:

1. A manipulator device comprising:

a base;

a first linear slide mounted to the base, the first linear slide having a first carriage movable along a first axis;

a second linear slide mounted to the first carriage, the second linear slide having a second carriage movable along a second axis orthogonal to the first axis;

a drive link coupled between the base and the second carriage, the drive link being rotatable about a proximal center of motion that is fixed relative to the base, the drive link being configured to move the second carriage in an arcuate path relative to the base, the arcuate path having a constant radius, wherein the first and the second linear slides constrain the second carriage to have a non-rotating orientation relative to the base as the second carriage moves along the arcuate path;

a drive member carried by the second carriage and connected to the drive link such that the drive member rotates with respect to the second carriage as it moves along the arcuate path but maintains the same rotational orientation as the drive link;

a driven member carried by the second carriage, the driven member being laterally spaced apart from and rotationally coupled to the drive member such that the driven member rotates with respect to the second carriage as it moves along the arcuate path but the driven member maintains the same rotational orientation as the drive member and the drive link; and

an end effector carried by the second carriage and rotationally coupled to the driven member such that the end effector maintains the same rotational orientation as the driven member, the drive member, and the drive link, the elements of the manipulator device thereby cooperating to constrain the end effector to rotate about a remote center of motion that is displaced from the proximal center of motion as the drive link moves the second carriage along the arcuate path.

8

2. The manipulator device of claim **1**, wherein the base is rotatable about an axis that intersects the proximal center of motion and the remote center of motion such that the end effector is spherically rotatable in two degrees of freedom about the remote center of motion.

3. The manipulator device of claim **2**, wherein the device further comprises shaft encoders to provide feedback of rotational positions in the two degrees of freedom about the remote center of motion.

4. The manipulator device of claim **1**, further comprising a prime mover coupled to the drive link and configured to move the second carriage along the arcuate path.

5. The manipulator device of claim **4**, wherein the device includes an automated mode in which at least one degree of freedom is driven by a computer controlled actuator.

6. The manipulator device of claim **1**, wherein the end effector is configured to be manually moved, and the drive link is configured to follow the motion of the second carriage and constrain the second carriage to move along the arcuate path.

7. The manipulator device of claim **6**, wherein the device includes a powered assist mode in which manual movements of the end effector are sensed and a prime mover provides force to assist with those movements.

8. The manipulator device of claim **7**, wherein the device includes the manual mode, the powered assist mode, and an automated mode in which at least one degree of freedom is driven by a computer controlled actuator.

9. The manipulator device of claim **1**, wherein the end effector comprises an intravenous line inserter.

10. A method of constraining an end effector to rotate about a remote center of motion that is displaced from a proximal center of motion that is fixed relative to a base, the method comprising:

providing the base and a first linear slide mounted to the base, the first linear slide having a first carriage;

moving the first carriage along a first axis;

providing a second linear slide mounted to the first carriage, the second linear slide having a second carriage;

moving the second carriage along a second axis orthogonal to the first axis;

providing a drive link coupled between the base and the second carriage;

rotating the drive link about the proximal center of motion such that the drive link moves the second carriage in an arcuate path relative to the base, the arcuate path having a constant radius, wherein the first and the second linear slides constrain the second carriage to have a non-rotating orientation relative to the base as the second carriage moves along the arcuate path;

providing a drive member carried by the second carriage and connected to the drive link;

rotating the drive member with respect to the second carriage as it moves along the arcuate path and maintaining the same rotational orientation as the drive link;

providing a driven member carried by the second carriage, the driven member being laterally spaced apart from and rotationally coupled to the drive member;

rotating the driven member with respect to the second carriage as it moves along the arcuate path and maintaining the driven member in the same rotational orientation as the drive member and the drive link; and

providing an end effector carried by the second carriage and rotationally coupled to the driven member such that the end effector maintains the same rotational orientation as the driven member, the drive member, and the drive link.

11. The method of claim 10, further comprising rotating the base about an axis that intersects the proximal center of motion and the remote center of motion such that the end effector is spherically rotated in two degrees of freedom about the remote center of motion. 5

12. The method of claim 11, further comprising providing feedback with shaft encoders of rotational positions in the two degrees of freedom about the remote center of motion.

13. The method of claim 10, further comprising moving the second carriage along the arcuate path with a prime mover coupled to the drive link. 10

14. The method of claim 13, further comprising selecting an automated mode of the device in which at least one degree of freedom is driven by a computer controlled actuator.

15. The method of claim 10, further comprising manually moving the end effector, and allowing the drive link to follow the motion of the second carriage and constrain the second carriage to move along the arcuate path. 15

16. The method of claim 15, further comprising selecting a powered assist mode of the device in which manual movements of the end effector are sensed and a prime mover provides force to assist with those movements. 20

17. The method of claim 16, further comprising alternately selecting between the manual mode, the powered assist mode, and an automated mode of the device in which at least one degree of freedom is driven by a computer controlled actuator. 25

18. The method of claim 10, further comprising providing an intravenous line inserter on the end effector.

* * * * *

30